

Original Research Article

Calibration of Inductive Electromagnetic Meter for Determining Electrical Conductivity of UAS, Raichur soil

Abstract

EM-38 electromagnetic induction sensor is most useful instrument to determine the soil salinity. Significant positive correlation found between inductive electromagnetic meter (IEM) readings and saturated paste extract electrical conductivity (EC) revealed that this technique can be used for determination of soil salinity. However, calibration of instrument is necessary for interpretation of instrument readings in terms of meaningful parameters of soil salinity. The calibration equations developed elsewhere may not predict electrical conductivity of UAS, Raichur soil accurately. So, in this study, calibration of EM-38 was carried out to find the soil salinity of UAS, Raichur soil. Multiple linear regression equation was developed which valid up to 20 cm depth after calibration of the instrument for UAS, Raichur soil and this equation considered reliable as it shows significant positive correlation between predicted and measured soil salinity values. Co-efficient of determination (R^2) between predicted and measured EC values was found to be 0.817. While salinity measurements made with the EM-38 are not highly accurate, but measurements within reasonable accuracy can be made very rapidly. Hence, this equation enables the user of the EM-38 to derive a realistic index of salinity of soil under consideration in terms of EC.

Keywords: Soil salinity, Soil electrical conductivity, EM-38, Electromagnetic Induction.

1. Introduction

Irrigation is essential in arid and semi-arid regions for agricultural production. However, it should be noted that soil salinity may be a risk for sustainable agricultural production owing to

mismanagement of irrigation schemes and other inherent problems of irrigation methods. Salt accumulation which may occur in plant root zone may closely be associated with the irrigation methods used. Irrigation with inferior quality of water may also increase soil salinity and it is one of the major pollutants which affect the crop yield and consequently the economic condition of farmers.

Soil salinity assessment with respect to area, severity and spatial variability is inevitable for the management and reclamation especially in canal commands, where salinity is one of the major constraints for crop production. Hence, the assessment of extent of soil salinity in irrigation command areas is necessary.

Traditional method of electrical conductivity measurement in saturation paste is laborious and time consuming as it requires extensive soil sampling and laboratory analysis. Therefore, there is a need to standardize the methods which should be rapid, non-destructive and measure the soil salinity directly in the field, without the involvement of any laboratory procedure. During the last two decades many new techniques like Wenner Array (Rhoades and Ingvalson, 1971), Rhoades's electrical conductivity probe (Rhoades, 1976), Time Domain Reflectometry (TDR) and Electromagnetic Induction (McNeill, 1980a and 1980b) have been developed to measure the in-situ soil salinity. In India, EM-38 meter was calibrated for black soils of Upper Krishna Project command in which coefficient of determination (R^2) between predicted and measured EC values were ranged between 0.79 to 0.89 (Kuligod, V.B. et. al, 2001).

Electromagnetic induction (EMI) meters have been shown to be effective for accurately and rapidly diagnosing and mapping the spatial distribution of subsurface soil salinity (Corwin and Lesch, 2003). The meters detect the apparent electrical conductivity of soil by measuring the response of the soil to an induced EM field. Electromagnetic induction technique is more

convenient and faster because its measurements do not require soil sampling and their preparations. An instrument named EM-38, which worked on the principle of EMI (Electromagnetic Induction), is commercially available which can be used to measure soil salinity. Utilization of an EM-38 meter seems to be cost effective method for assessing field salinity and for experiments on salt tolerance of crops.

In saline soils, salt dominates the response of the EM meter and generally good correlations have been found between apparent soil electrical conductivity (ECa) and salinity (de Jong et al., 1979; Cameron et al., 1981; Williams and Baker, 1982). So, EM-38 records readings proportionate to the amount of salts in soil. Also, EM-38 does not require direct soil penetration; therefore a large number of readings can be taken at much lower cost than conventional soil sampling. It can be used to measure soil salinity to approximately 0.6 to 1.2 m depth depending on the orientation of meter.


Keeping all above points in mind, present study was carried out to calibrate the EM-38 meter and develop a multiple linear regression equation to determine the soil salinity of UAS, Raichur area accurately and at faster rate.

2. Materials and Methods:

2.1 Working Principle of EM-38:

The schematic diagram of EM-38 is presented in Fig. 1 which is showing the location of two electrical coils i.e. transmitter coil (Tx) and receiver coil (Rx), placed one meter apart. Transmitting coil creates a primary magnetic field (H_p) and this magnetic field generates eddy current in ground. This eddy current loop induces its own magnetic field (H_i) in soil. Ratio of H_p and H_i are measured by receiver coil and this ratio is proportional to electrical conductivity of soil.

71

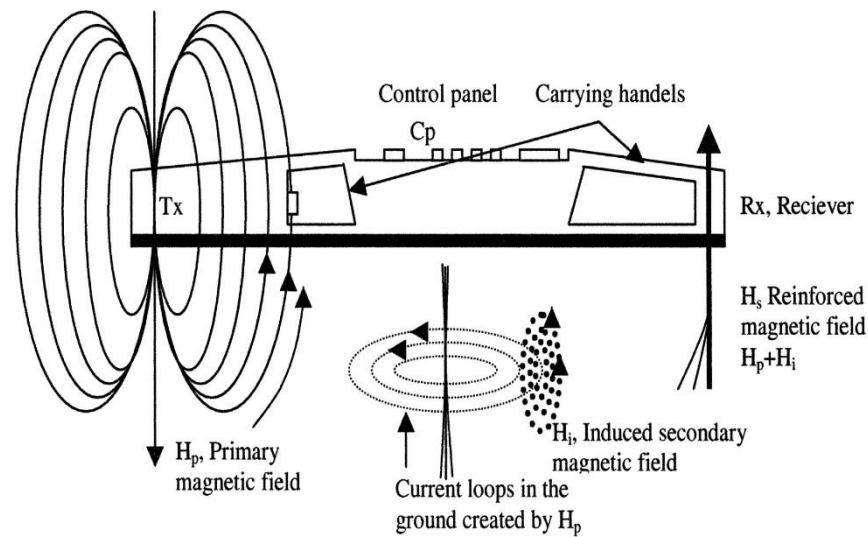

72

73

Fig. 1. Schematic diagram of EM-38 showing working principle.

74 2.2 Study Area:

75 The experimental site is located in the UAS, Raichur campus comprises block No. 87 to 107 of
 76 agricultural land in Raichur district of Karnataka, India. This area is situated in the north eastern
 77 dry zone of Karnataka located at 16°21'N latitude, 76°24'E longitude and 389.5mm above mean
 78 sea level. The daily climatological data during the period of study were recorded from the
 79 metrological station at the regional research station, Raichur. It is seen that the maximum
 80 temperature of 43.3°C was recorded in the month of May and the minimum temperature of 20°C
 81 was recorded in the month of January. The maximum average relative humidity of 78.5% was
 82 recorded in the month of January and minimum of 23.5% was recorded in the month of March.
 83 The maximum wind velocity of 21.2 km per hour was in the month of February. The maximum
 84 evaporation of 16.5 mm/day was in the month of May and the minimum evaporation of 2.0
 85 mm/day was in the month of January.

86 2.3 Soil salinity data collection:

87 2.3.1 Setting procedure of EM-38:

Before using EM-38 for taking readings, initial phase nulling of EM-38 is required to facilitate the receiver coils to measure the very small signal from eddy currents in presence of the much larger signal arising from the primary magnetic field. Fig. 2 shows the various knobs present on EM-38 for nulling operation which should carried out prior to calibration.

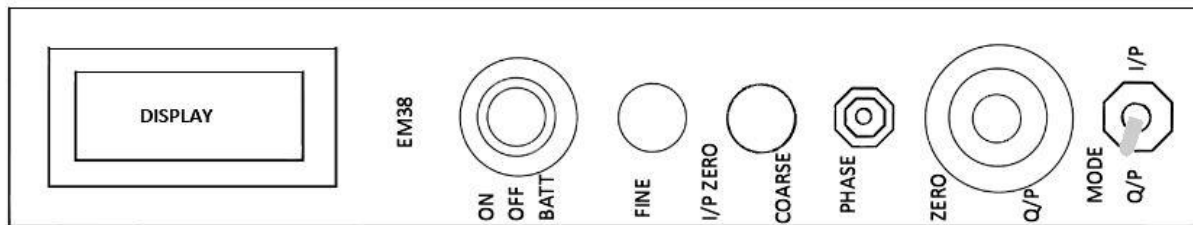


Fig. 2. Knobs present on EM-38 for nulling operation.

Step 1: Place EM-38 on the ground and flip switch to Q/P. Notice the reading in display and make it zero using the Q/P knob.

Step 2: Flip switch to I/P. Make the reading zero using I/P knobs. We can use coarse as well as fine both knobs for adjustment.

Step 3: Again flip switch back to Q/P. Make the reading zero using Q/P knob.

Step 4: Now, lift the EM-38 to about five feet above the ground. The black bar along the bottom of the meter should be pointing out to the horizon. Reset meter as did in Steps 1-3 with the meter still pointed to the horizon.

2.3.2 Data Collection:

The data was collected from block No. 87 to 107 of UAS, Raichur campus. For taking readings using EM-38, place the EM-38 horizontally and record the reading, H. Then, place it vertically

and record the reading, V. Collect the soil sample from same place to determine the electrical conductivity of soil of that point in laboratory.

2.4 Data Analysis:

After collection of data i.e. H and V values and finding out electrical conductivity (EC) of collected soil samples in laboratory, it was necessary to analyses data whether dependent variable i.e. electrical conductivity depend on independent variables i.e. H and V values. Fig. 3 shows the graph between electrical conductivity and horizontal values. The coefficient of determination (r^2) is 0.7182 which is on higher side. So, we can say that electrical conductivity depends on horizontal values which we obtained using EM-38. Similarly, Fig. 4 shows the graph between electrical conductivity and vertical values. The coefficient of determination (r^2) is 0.726 which suggest that electrical conductivity does depend on vertical values too.

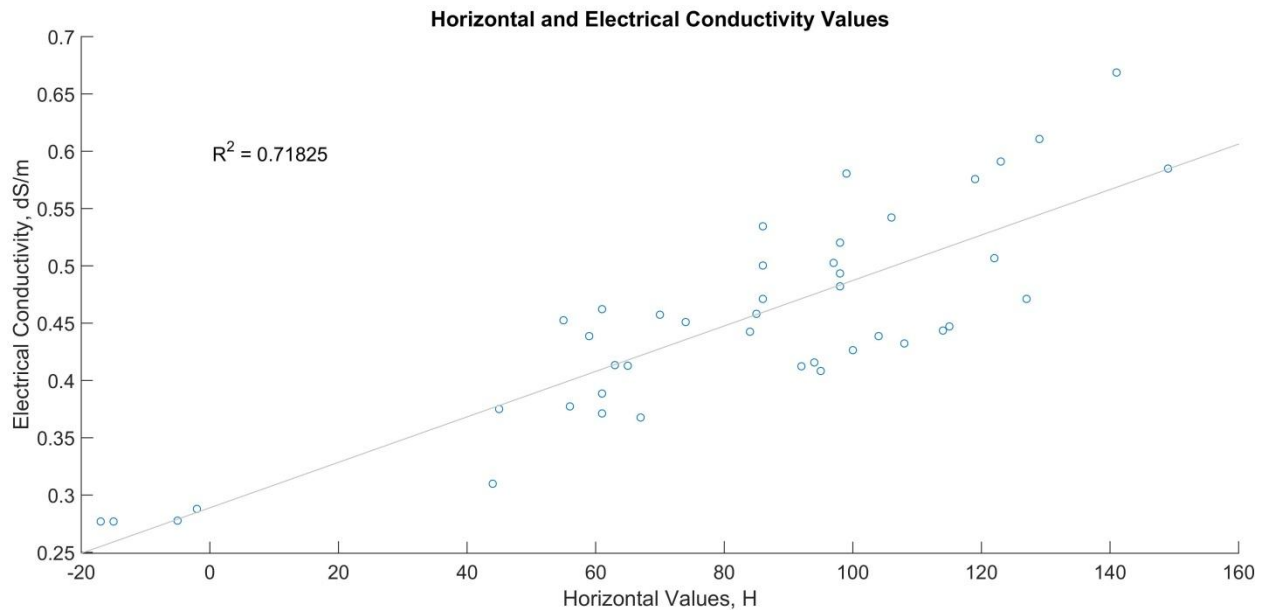


Fig. 3. Graph to show electrical conductivity depends on Horizontal values.

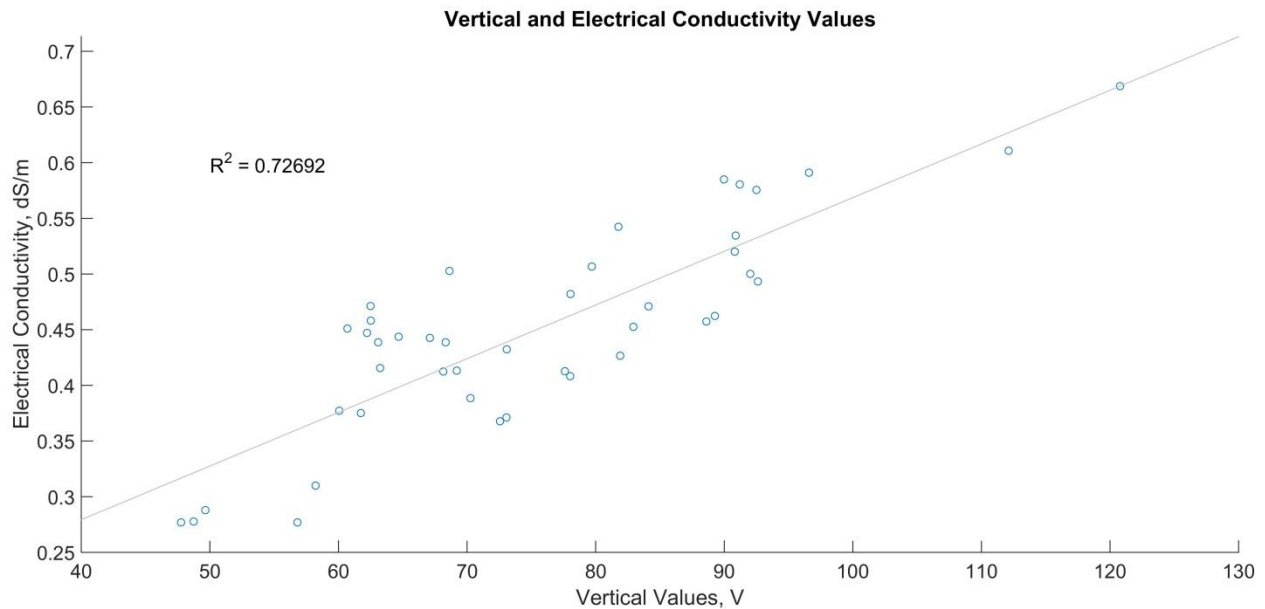


Fig. 4. Graph to show electrical conductivity depends on vertical values.

Multicollinearity is a condition in which independent variables in a regression model are correlated. Multicollinearity condition between independent variables also checked in this study because presence of multicollinearity reduces the precision of estimate coefficients, which weakens the statistical power of regression model. Fig. 5 shows the graph between horizontal and vertical values and their coefficient of determination (r^2) is 0.425. From this, we can say that vertical and horizontal values are not highly correlated and hence multicollinearity is not present in this case.

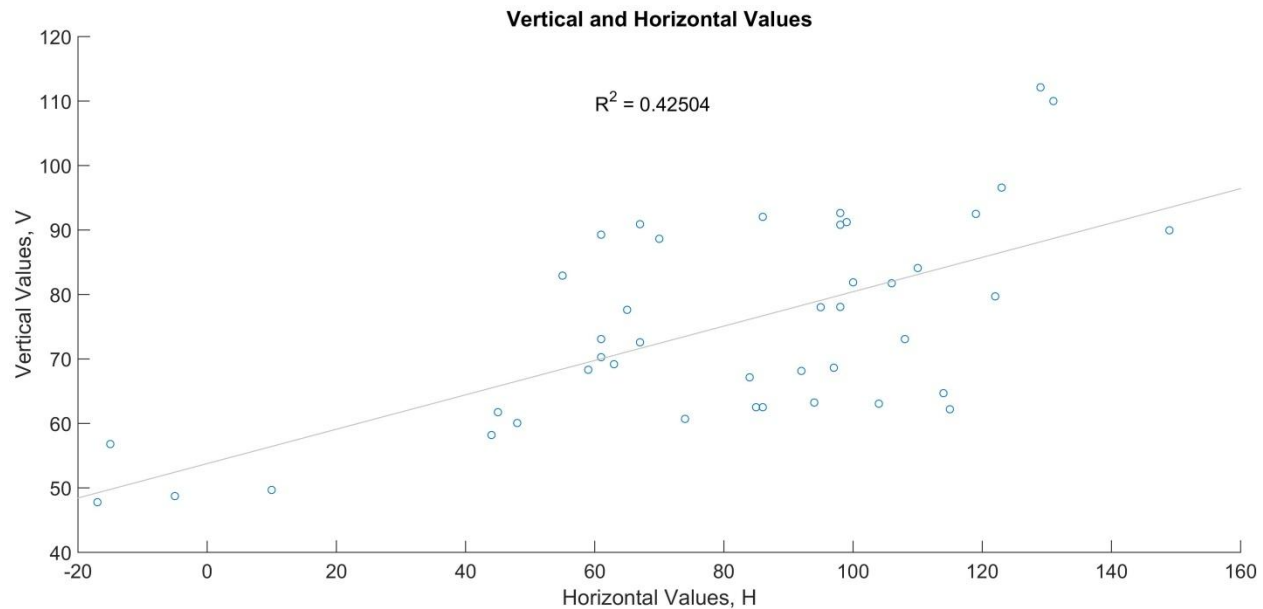


Fig. 5. Multicollinearity between horizontal and vertical values.

3. Results and Discussion:

3.1 Development of predictive equation:

Field data (H and V readings along with respective EC) valued were subjected to multiple linear regression analysis. New predictive equation was developed for depth of 0-20 cm using EM-38 data. Up to 20 cm depth is considered for this study because tillage operations usually performed up to 20 cm only. Table 1 show the output estimated coefficients obtained from multiple regression analysis. In Table 1, it observed that after conducting t-test, p-value of each predictor is less than 0.0001 at significance level of 5%.

Table 1. Estimated coefficients obtained from multiple linear regression analysis.

	<i>Coefficients</i>	<i>Standard Error</i>	<i>t Stat</i>	<i>P-value</i>	<i>Lower 95%</i>	<i>Upper 95%</i>
Intercept	0.134103	0.026239	5.110819	8.31E-06	0.081072	0.187134
H	0.001176	0.000182	6.473375	1.02E-07	0.000809	0.001543
V	0.002919	0.000438	6.657588	5.64E-08	0.002033	0.003805

The multiple linear regression equation to predict EC with coefficient of determination (R^2) is shown in Table 2. As the coefficient of determination is more than 0.80 so we can say that this

equation is able to predict EC accurately at faster rate as compare to conventional laboratory method.

Table 2. Developed equation and coefficient of determination.

Depth, cm	Equation used	No. of samples	R ²
0-20	$0.00117(H) + 0.00292(V) + 0.134$	43	0.824

To examine the quality of the fitted model, ANOVA is conducted on collected data as shown in Table 3. From Table 3, it observed that the effects of H and V in model are significant as p-value is less than 0.05 for both variables.

Table 3. Summary of ANOVA

	SS	DF	MS	F	p Value
H	0.048484	1	0.048484	41.36	1.17E-07
V	0.051511	1	0.051511	43.942	6.19E-08
Error	0.04689	40	0.001172		

3.2 Regression Model Evaluation:

Adequacy of a regression model was determined using residual analysis (residuals uncorrelated and normally distributed with zero mean and a constant variance (Montgomery and Peck, 1982). All statistical analyses required for model evaluation were performed using MATLAB 2014b. Significance was reported at a probability level of 0.05. The histogram of residual can be used to check whether the variance is normally distributed or not. Fig. 6 shows the histogram of residuals. A symmetric bell-shaped histogram which is evenly distributed around zero indicates that the normality assumption is likely to be true.

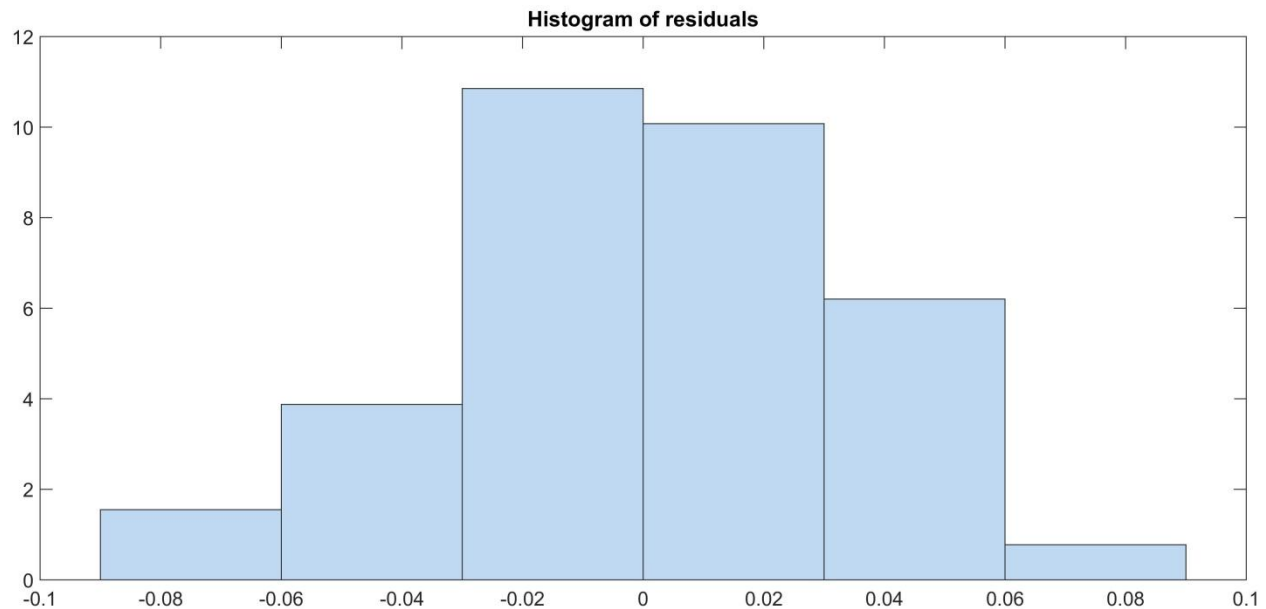


Fig. 6. Histogram of residuals.

A normal probability plot of residuals also be used in this study to check whether the variance is normally distributed or not. If the resulting plot is approximately linear, we can proceed assuming that the error terms are normally distributed. As shown in Fig. 7 residuals are lying on line so we can say that variance is normally distributed.

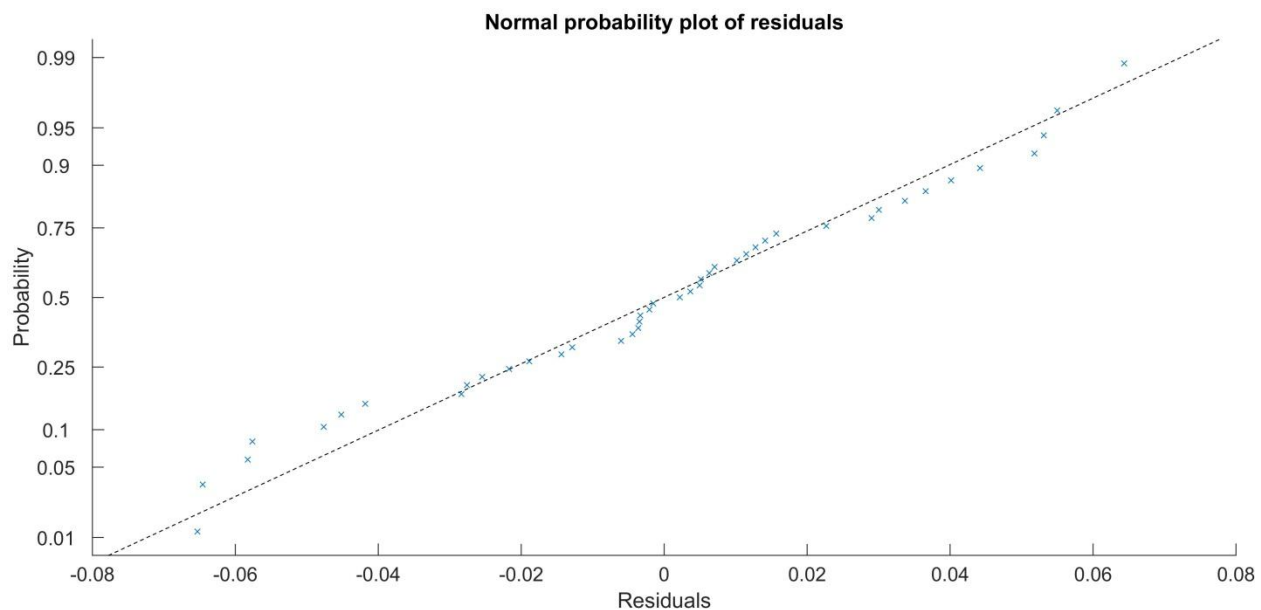


Fig. 7. Normal probability plot of residuals.

169 The residual error log plot, constructed by plotting residual (i) against residual (i-1) is useful for
 170 examining the dependency of error terms on each other. Any non-random pattern in a plot
 171 suggests that variance is non-random. As shown in Fig. 8, the pattern is random which suggest
 172 that the variance is random and error terms are not related with each other.

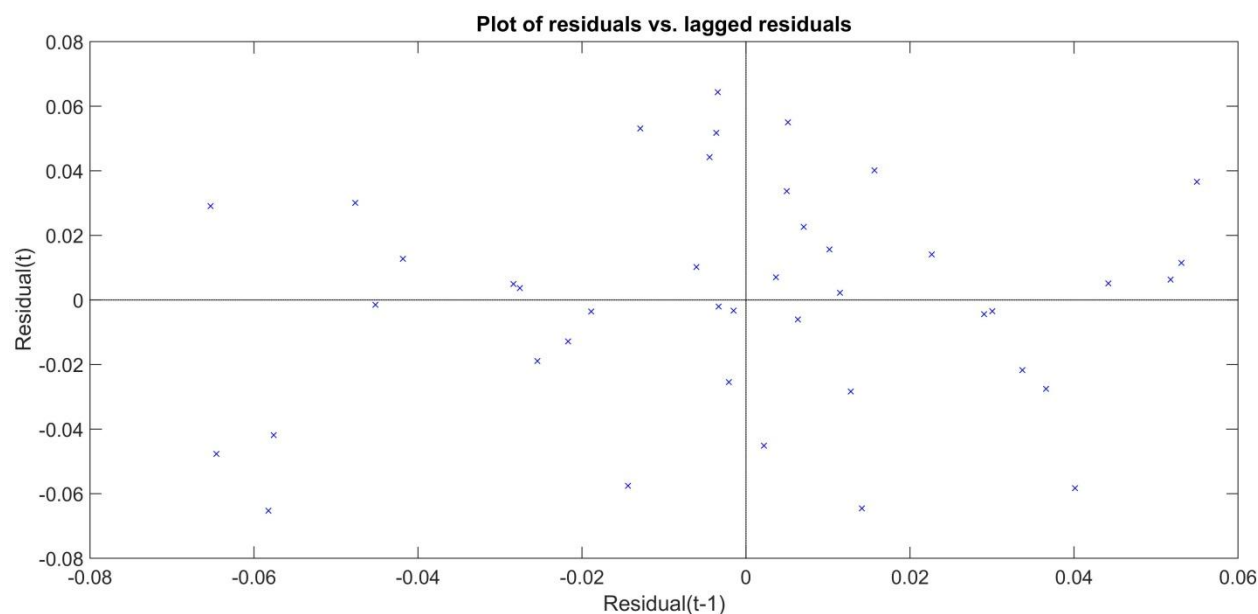


Fig. 8. Residual vs lagged residual graph.

175 Residual case order plot was used to find out outlier points. As shown in Fig. 9 the interval
 176 around all the residual does contain zero. This indicates that the residual is smaller than expected
 177 in 95% of observations and it suggests that there were no outlier data points.

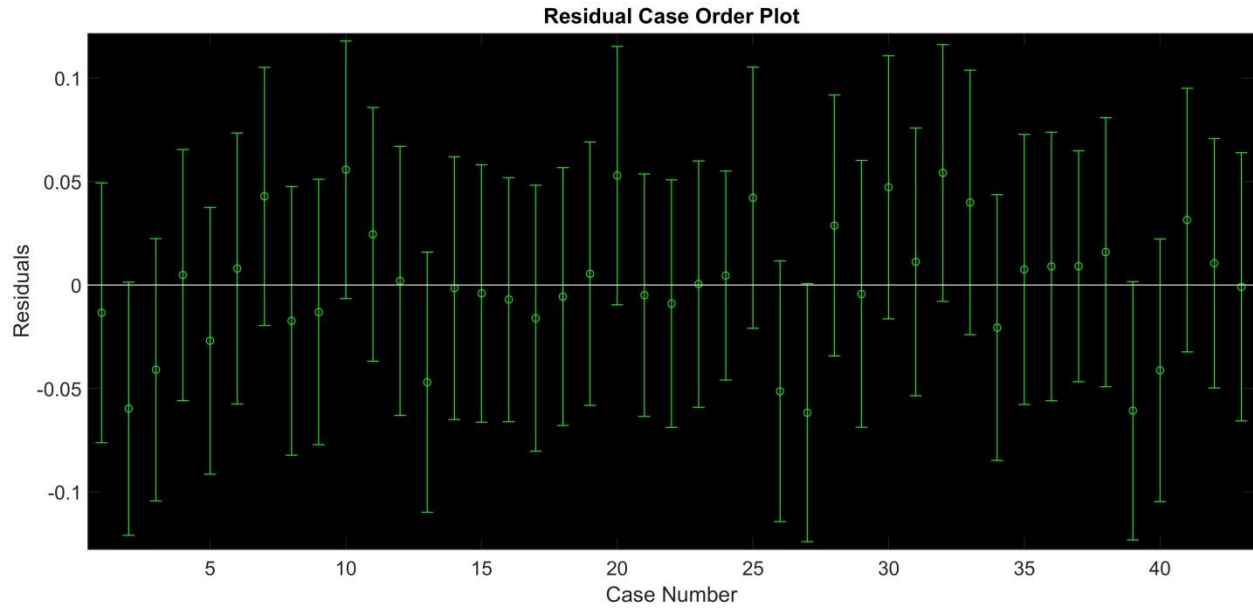


Fig. 9. Residual case order plot to find outlier data points.

Fig. 10 shows the 3D plot between collected data and EC. Variation in EC is shown using 3D surface with color map bar.

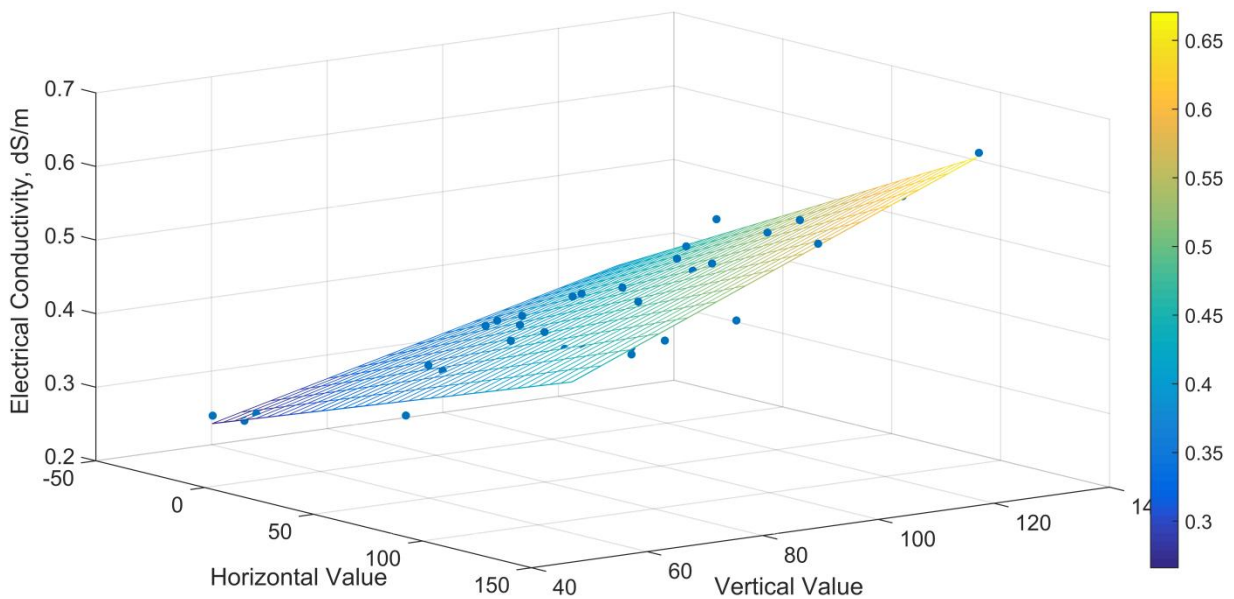


Fig. 10. Plot between collected data and EC.

To evaluate the accuracy and precision of suggested multiple linear regression model, 20 readings were taken using EM-38 and electrical conductivity of soil was found out in laboratory

for the same places. Using model, electrical conductivity of soil at these points were predicted and graph was plotted between predicted and actual electrical conductivity as shown in Fig. 11. From Fig. 11, it observed that the coefficient of determination (r^2) is 0.817. Therefore, model proposed in this study can be used to predict electrical conductivity of UAS, Raichur soil.

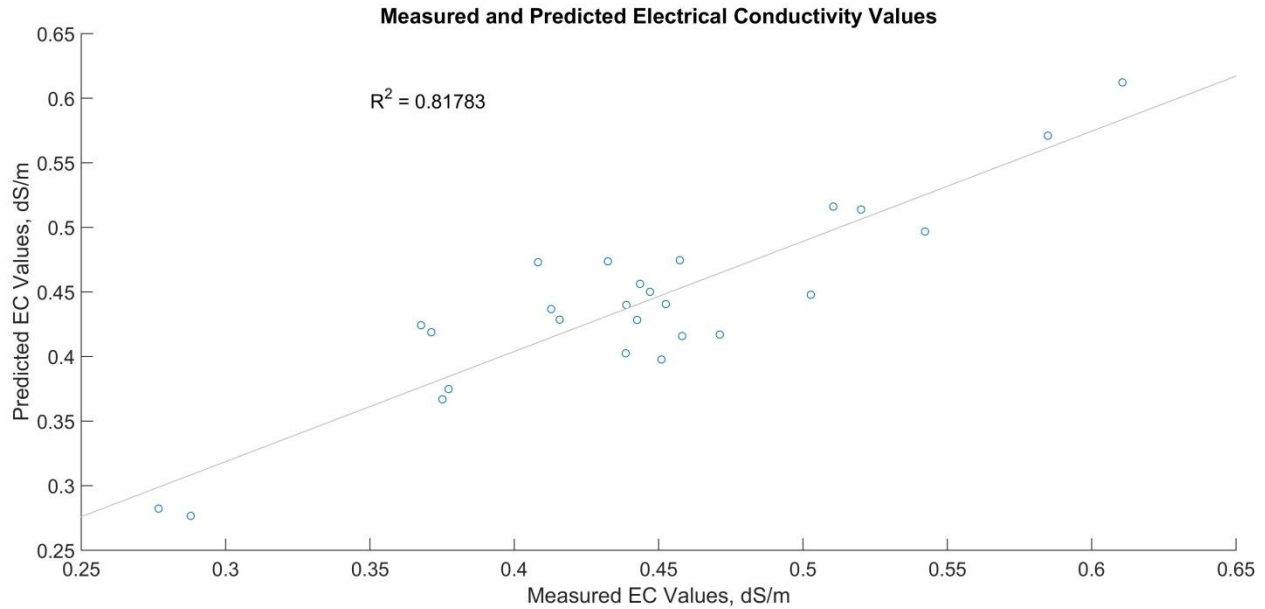


Fig. 11. Plot of measured and predicted EC values.

4. Conclusions:

The objective of this paper was to infer the soil salinity value of UAS, Raichur soil using EM-38 meter as this meter able to infer salinity rapidly without any post processing of soil sample in laboratory. Before using EM-38, its calibration is required to decrease errors in predicted soil salinity. Multicollinearity was not found between independent variables as r^2 value was 0.425. Also, high correlation was obtained when electrical conductivity values were plotted against horizontal values ($r^2 = 0.718$) and vertical values ($r^2 = 0.727$). Therefore, both values contributed significantly in prediction of electrical conductivity of soil. Normal probability plot of residuals shows that variance is normally distributed and error terms are independent with each other as

find out from plot of residuals vs lagged residuals. Co-efficient of determination (R^2) between predicted and measured values of electrical conductivity was 0.817. Hence, proposed equation enables the user of EM-38 to derive a realistic index of soil salinity in terms of electrical conductivity.

References:

- [1] Rhoades, J.D. and Ingvalson, R.D. 1971. Determining salinity in field soils with soil resistance measurements. *Soil Science Society of America Proceedings*, 35: 54-60.
- [2] Rhoades, J.D. 1976. Measuring, mapping and monitoring field salinity and water depths with soil resistance measurements. *FAO Soils Bulletin*, 31: 69-109.
- [3] McNeill, J.D. 1980a. Electrical conductivity of soil and rocks. Technical note TN-5 Geonics Ltd. Mississauga, Ontario, Canada, pg.21
- [4] McNeill, J.D. 1980b. Electromagnetic terrain conductivity measurements at low induction numbers. Technical note TN-5 Geonics Ltd. Mississauga, Ontario, Canada, pg.15
- [5] Kuligod, V.B., Salimath, S.B., Vijayashekhar, K., Balakrishnan, P., 2001. Calibration of Inductive Electromagnetic Meter for Determining Electrical Conductivity in Vertisols. *J. of Indian Society of Soil Science*. 49, 479-482.
- [6] Corwin, D.L., Lesch, S.M., 2003. Application of soil electrical conductivity to precision agriculture: theory, principles, and guidelines. *Agron. J.* 95, 455–471.
- [7] De Jong, E., Ballantyne, A.K., Cameron, D.R., Read, D.W.L., 1979. Measurement of apparent electrical conductivity of soils by an electromagnetic induction probe to aid salinity surveys. *Soil Sci. Soc. Am. J.* 43, 810–812.
- [8] Cameron, D.R., de Jong, E., Read, D.W.L., Oosterveld, M., 1981. Mapping salinity using resistivity and electromagnetic inductive techniques. *Can. J. Soil Sci.* 61, 67–78.
- [9] Williams, B.G., Baker, G.C., 1982. An electromagnetic induction technique for reconnaissance surveys of soil salinity hazards. *Aust. J. Soil Res.* 20, 107–118.
- [10] Montgomery, D. C., and E. A. Peck. 1982. *Introduction to Linear Regression Analysis*. New York, N.Y.: John Wiley and Sons.