

Comparative analysis of molecular methods for detection of Influenza viruses.

ABSTRACT

Aims: Influenza is a serious threat to human population worldwide therefore continuous surveillance is required to update influenza seasonal vaccines. A rapid, sensitive, specific and cost effective diagnostic method will be much helpful for patient management in the present scenario. Present study is conceptualized for detection of influenza viruses by molecular methods and compare with 'gold standard' virus isolation.

Study Design: Standard strains of Influenza virus were used to standardize the molecular diagnostic assays and results were then compared with virus isolation.

Place and Duration of Study: Centre for Biotechnology, Maharshi Dayanand University, Rohtak, Haryana, India, between December 2015 and April 2016.

Methodology: Standard strains of Influenza A and B virus were used for influenza virus isolation using virus culturing in MDCK (Madin-Darby Canine Kidney) cell line by following standard tissue culture procedure. Isolated viruses were detected by Hemagglutination assay (HA) and typed by Hemagglutination inhibition assay (HI). Conventional one step RT-PCR, Taqman real time RT-PCR and RT-LAMP (Reverse transcription loop mediated isothermal amplification) were standardized on RNA extracted from standard strains. Sensitivity and specificity of these molecular methods were compared with each other as well as with virus culture (gold standard).

Results: Both influenza A and B virus strains were cultured in MDCK cells and produced cytopathic effect during virus culture. Conventional RT-PCR and real time RT-PCR detected both type of Influenza viruses. RT-LAMP also successfully detected and typed influenza viruses. RT-LAMP proved to be more rapid than other two molecular assays.

Conclusion: Molecular diagnostic methods are useful in detection and typing of Influenza viruses and these methods provide results in short period of time when compared with traditional virus culture methods. RT-LAMP is rapid, sensitive, specific and cost effective method for influenza virus detection and subtyping.

Key words: *Influenza Virus; Conventional one step RT-PCR; Taqman real time RT-PCR; RT-LAMP.*

Abbreviations: *PFU: Plaque forming units; TPCK: Tosyl phenylalanyl chloromethyl ketone; PCR: Polymerase chain reaction; DMEM: Dulbecco's Modified Eagle's medium; FBS: Fetal bovine serum; BSA: Bovine serum albumin.*

1. INTRODUCTION

Influenza viruses are mainly accountable for respiratory illness and significant loss of human lives worldwide. There are many epidemics and pandemics due to Influenza viruses and causes of high morbidity and mortality in humans and other organisms. Influenza pandemics are very old and at least about thirty one times have been recorded since the last 400 years [1]. Influenza viruses (family *Orthomyxoviridae*) are characterized by a segmented, minus--single stranded RNA genome. Influenza viruses are irregular in shape, spherical (80-120 nm diameter) or filamentous structures and their surfaces are marked with rod-shaped hemagglutinin (HA) and neuraminidase (NA) spikes [2]. Influenza viruses can be further typed into A, B and C based on the antigenic differences in the nuclear and matrix proteins. Fourth type of Influenza virus (type D) is proposed recently and is related to bovine infections [3-5]. Influenza A viruses are further sub-typed according to the antigenicity of their surface glycoprotein HA and NA [6]. Eighteen (~~H1-H18~~) different hemagglutinin subtypes (H1-H18) and eleven (~~N1-N11~~) different neuraminidase subtypes (N1-N11) are detected so far. H1N1 and H3N2 strains are prevalent among human population on seasonal basis [7]. Almost all sub-types of HA and NA have been isolated from aquatic birds as these are the natural host to the viruses [8-9]. Influenza A viruses show more antigenic variability due to antigenic drift and shift phenomenon which may cause both epidemics and pandemics due to influenza. Influenza B viruses show lesser antigenic variation resulting in epidemics whereas influenza C viruses have limited clinical significance [10-11]. New strains of the Influenza A viruses with human infection potential constantly appear due to this drift and shift, like the new avian influenza A (H7N9) virus [12]. Thus influenza affects a large segment of world population resulting in high mortality, morbidity and economic loss. World health organization (WHO) has estimated that globally, about 3-5 million cases of hospitalization and 250,000 to 500,000 deaths occur due to Influenza every year [13]. Considering the impact of influenza on the health, WHO has established an Influenza surveillance network to collect influenza virus isolates and epidemiological data. At present, five WHO collaborating centres are in Atlanta, Beijing, London, Melbourne, Tokyo and 136 National Influenza Centers (NIC) are located in 106 countries [14]. These centres are working in collaboration with each other on continuous surveillance of Influenza virus and provide the data for effective vaccine development against current circulating strains of influenza viruses. Laboratory diagnosis for influenza virus can be by virus isolation in chicken egg embryo or cell culture, antigenic and serological analysis [15], rapid detection kits as well as molecular detection methods based on nucleic acid amplification like NASBA (nucleic acid sequence based amplification) [16], conventional reverse transcription PCR [17-18]. Latest molecular diagnostic methods include Real-time RT-PCR [19-20], DNA Microarray based tests [21-22] and reverse transcription loop mediated isothermal amplification (RT-LAMP) [23-25]. Rapid, sensitive, specific and cost effective methods are required for surveillance, best patient management and virus outbreaks prevention. The present study is conceptualized to detect influenza viruses by nucleic acid based

methods (conventional RT-PCR, real time RT-PCR, RT-LAMP), in comparison with gold standard i.e. virus culture.

2. METHODOLOGY

2.1 Standard Strains of Influenza virus and MDCK cell line

The standard strains of Influenza A (A/New Caledonia/20/99 (H1N1-like) and Influenza B (B/Hong-Kong/330/2001) viruses and stocks of Madin-Darby Canine Kidney (MDCK) cell lines were kindly provided by Department of Microbiology, AIIMS, New Delhi, India.

2.2 Virus culture

Virus isolation can be done in both chicken egg embryo and cell culture; however egg culture has certain disadvantages like availability of large number of embryonated eggs, presence of other infective agents/pathogens and highly labour intensive. Therefore, we have used MDCK cell line of low passage level (up to #20) for virus culture. Tissue culture flasks having confluent monolayer of MDCK cells were used for growth of influenza viruses. Before inoculation, growth medium (DMEM with 10% FBS) was removed and cells were washed once with phosphate buffer saline (PBS) and twice with virus growth medium (VGM) (serum free DMEM with 2 µg/ml TPCK treated trypsin and BSA 150 mg/ml). Five hundred (500 µl) micro liters of appropriate dilution of each prototype strain of influenza virus ~~was~~ were inoculated into respective culture flask. Inoculum was allowed to adsorb for 30 minutes at 37 °C, followed by addition of 5-6 ml of serum free, virus growth medium to each flask. Flasks were incubated at 37 °C and observed daily for cytopathic effect (CPE). Flasks were harvested either when 3+ or 4+ CPE (more than one large patch per field of observation) was observed or on seventh day even if no CPE was observed. Presence of influenza virus and its titre was detected by Hemagglutination assay (HA). Hemagglutination inhibition assay (HI) was done to detect the type of influenza virus.

2.3 RNA extraction and aliquots

Viral RNA was extracted from an aliquot of standard strains of influenza virus using commercial GeneJET Viral DNA/RNA Purification Kit (Thermo Fisher Scientific, USA) following the manufacturer's instructions. RNA was eluted in a final volume of 50 µl in elution buffer (provided with kit) and divided into aliquots of 5 µl ~~each and for storage~~ aged at -80 °C until used.

2.4 Standardization of Conventional one-step Reverse transcription (RT-PCR)

One step RT-PCR was standardized with extracted RNA using Verso 1-Step RT-PCR Kit (Thermo Fisher Scientific, USA) using manufacturer's instructions. Separate reactions were standardized for detection of Influenza A and Influenza B virus. For Influenza A virus, primers were taken from the Matrix gene (M gene) as given by WHO [26]. Nucleoprotein gene (NP gene) was targeted for primer pairs to detect Influenza B virus (Table 1). Reaction mixture was comprised of 12.5_μl of 2× RT-PCR buffers, 1_μl of RT enhancer (provided with kit), 0.2_μmol/L of both forward and reverse primers, 0.5_μl of enzyme mix (Reverse Transcriptase (RT) and Taq polymerase) and RNase free water to make a final volume of 20_μl.

Table 1. Primers used in standardization of conventional one step RT-PCR for detection of Influenza A and B viruses.

Primer	Sequence (5'→3')	Target Gene	Amplicon Size (bp)
Inf A-Forward	AGTCTTCTAACCGAGGTCGAAACG	Matrix gene (M)	239
Inf A-Reverse	TGGACAAAGCGTCTACGCTGCA		
Inf B-Forward	ACGGTATCAACACTGGGACA	Nucleoprotein gene (NP)	198
Inf B-Reverse	TCGGGGTCTGTTTCTTTTGG		

Five microliters of viral RNA ~~was-were~~ added to the test tube to make a final volume of 25_μl. Negative controls were also included which contain 5_μl of RNase free water in place of viral RNA. Reaction mixtures were incubated at 50_°C for 50 min (reverse transcription), 94_°C for 15 min (RT inactivation), then 40 cycles of PCR: ~~Each cycle comprised of~~ denaturation at 94_°C for 30 sec, annealing at 55_°C for 45 sec and extension at 72_°C for 1 min, ~~following by a-~~ After final extension at 72_°C for 7 min (Ref[d11]). ~~The~~ reactions were stored at 4_°C ~~and the -After completion of~~ RT-PCR, amplicons were visualized by ~~electrophoresis in~~ 2.5% (w/v) agarose gel ~~electrophoresis~~.

2.5 Development of Taqman One-Step Real-Time RT-PCR Assay

Viral RNA extracted from the standard strains of influenza was used to standardize the Taqman One-Step Real-Time RT-PCR Assay. The Influenza A primer/probe set is for universal detection of type A Influenza virus and it amplified a product of 105_bp in Matrix gene M1 of Influenza A viruses; ~~while~~ the Influenza B primer/probe set amplified a product of 102_bp in Nonstructural protein (NS) gene of Influenza B virus (Table 2).

Table 2. Primers and probes used in standardization of real time RT-PCR for Influenza A and B viruses. K, R and Y represent mixture of (G,T), (A,G) and (C,T) respectively.

Primers and Probes	Sequence (5'→3')	Target Gene	Amplicon Size (bp)
Influenza A Forward	GACCRATCCTGTACCTCTGAC	Matrix gene (M1)	105
Influenza A Reverse	AGGGCATTYTGGACAAKCGTCTA		
Influenza A Probe*	TGCAGTCCTCGCTCACTGGGCACG		
Influenza B Forward	TCCTCAAYTCACTCTTCGAGCG	Nonstructural Gene (NS)	102
Influenza B Reverse	CGGTGCTCTTGACCAAATTGG		
Influenza B Probe*	CCAATTCGAGCAGCTGAAACTGCGGTG		

*TaqMan® probes were labeled at the 5'-end with the reporter molecule 6-carboxyfluorescein (FAM) and with the quencher, Blackhole Quencher 1 (BHQ1) (Biosearch Technologies, Inc., Novato, CA) at the 3'-end.

A single-step Real-Time RT-PCR was carried out using SuperScript III Platinum One-Step RT-PCR system (AgPath-ID™ One-Step RT-PCR Kit, Applied Biosystems, ThermoFischer Scientific, USA). Two sets of primer/probe (Influenza A and B) in separate tubes/wells were used in RT-PCR. Each primer and probe was used at a final concentration of 40_{pm} and 10_{pm}, respectively. The 25_{μl} reaction comprised a combination 12.5_{μl} of 2~~×~~ master mixture, 1.5_{μl} of primer/probe mixtures, ~~and~~ 1_{μl} of 25~~×~~ enzyme mixture, ~~and~~ 5_{μl} of RNase free water ~~for every reaction.~~ Positive reaction included 5_{μl} of viral RNA ~~while same amount or 5_{μl} of RNase free water was added to for the negative reaction control.~~ The cycling parameters for Real-Time RT-PCR were: reverse transcription at 50_{°C} for 30 min; Enzyme activation at 95_{°C} for 15 min; 35 cycles of two step PCR amplification ~~for of two steps~~, 95_{°C} for 15 sec and 55_{°C} for 1 min. Fluorescence data was collected during the 55_{°C} (annealing) step (ref[d2]?).

2.6 Reverse Transcription loop-mediated isothermal amplification (RT-LAMP)

RT-LAMP is standardized for the detection of influenza viruses using viral RNA extracted from the standard strains of Influenza A and B viruses. The primers used for influenza A virus were taken from the matrix gene [23] and for influenza B virus primers were taken from the nucleoprotein gene [27]. The reaction was standardized using Loopamp RNA amplification kit (Eiken Chemical Co. Ltd, Japan) following the manufacturer's instruction. Reaction mixture was prepared in two different tubes ~~each~~ for influenza A and B virus respectively. Each reaction cocktail was made of 12.5_{μl} of 2~~×~~ reaction buffer,

0.5_μl of enzyme mix, 1_μl of each F3 and B3 primers (5 picomoles/L), 1 μl each FIP and BIP primers (40 picomoles/L) (**Table 3**) and RNase free water was added to make final volume 20_μl.

Table 3. Primers used in standardization of RT-LAMP. Influenza A primers were taken from Matrix gene and Nucleoprotein gene was targeted for Influenza B virus primers.

Primer	Type of Primer	Sequence (5'→3')	Primer length (bp)
Influenza A			
Inf A-F3	Outer forward primer	TGGTGCACCTTGCCAGTTG	18
Inf A-B3	Outer reverse primer	CCAGCCATCTGTTCCATAGC	20
Inf A-FIP	Inner forward primer	TGCTGTGAATCAGCAATCTGTTA CAGGATGGGAACAGTGACC	42
Inf A-BIP	Inner reverse primer	AGACAAATGGCTACTACCACCC GTAGTGCTAGCCAGCACC	40
Influenza B			
Inf B-F3	Outer forward primer	ACGGTATCAACACTGGGACA	20
Inf B-B3	Outer reverse primer	TCGGGGTCTGTTTCTTTTGG	20
Inf B-FIP	Inner forward primer	GCAAGGGTTGCTGGTCTAATGA ATTGACAAAACACCGGAAGA	42
Inf B-BIP	Inner reverse primer	CCCACCAAGCAACAAACGAACC CGACATCATCTTCACTGC	40

Five microliters of viral RNA was added to it-making a final reaction volume of 25_μl. Negative controls were also included. The reaction is incubated at 63_°C for 1 hour (amplification) and 80_°C for 15 min (enzyme inactivation). The amplicons were visualized on 2.5% (w/v) agarose gel electrophoresis.

2.7 Sensitivity and specificity of molecular assays

Standard strain of Influenza A virus (A/New Caledonia/20/99 (H1N1-like) with known viral titre (~~3×10~~³ PFU/μl) was used to compare the sensitivity of three molecular assays i.e. conventional RT-PCR, real time RT-PCR and RT-LAMP. The RNA was extracted from 100_μl of standard strain of influenza A virus using GeneJET Viral DNA/RNA Purification Kit (Thermo Fisher Scientific, USA) following the manufacturer's instructions and eluted in final volume of 50_μl. Final eluted viral RNA is supposed to have viral titre of 10³ PFU/μl. ~~Ten-fold serial-Decimal~~ dilutions of viral RNA were ~~made-prepared~~ in RNase free water. ~~Dilutions were made-ranging~~ from 10⁻¹ to 10⁻⁵ PFU/reaction and ~~these dilutions were then~~ used as

sample RNA in all three assays as described earlier. When dealing with RNA, care was taken to minimize freeze/thaw cycles and all the three molecular assays were setup on the same day to minimize viral RNA degradation.

Specificity of the molecular assays was checked against other viruses causing influenza like illness such as parainfluenza viruses, adenoviruses and Respiratory syncytial virus (RSV).

3. RESULTS AND DISCUSSION

A rapid, specific and sensitive method to detect influenza virus is much important for effective patient management and to early start of antiviral therapy. It also helps in surveillance of newly emerging influenza strains, vaccine development and to check the spread of virus in early stages, hence preventing epidemics or pandemics of influenza. Conventional methods like virus isolation using egg embryo culture, cell culturing, shell vial culturing, antigen detection and serological analysis are used for the laboratory diagnosis of influenza viruses [28]. In our study virus culture in MDCK cell line both influenza A and B viruses showed cytopathic effect (CPE) in MDCK cells on 4th days of post inoculation. CPE due to influenza virus in MDCK cells was seen as rounding and lacy appearance of cells (**Fig. 1**). ~~Presence of influenza viruses were detected by Hemagglutinin assay (HA).~~[d3] HA titers of ~~both the two~~ isolates were ~~found to be~~ 1:256 for influenza A and 1:64 for influenza B respectively. ~~Both isolates were typed by hemagglutinin inhibition assay (HI) using WHO influenza reagent kit and guidelines.~~[d4]

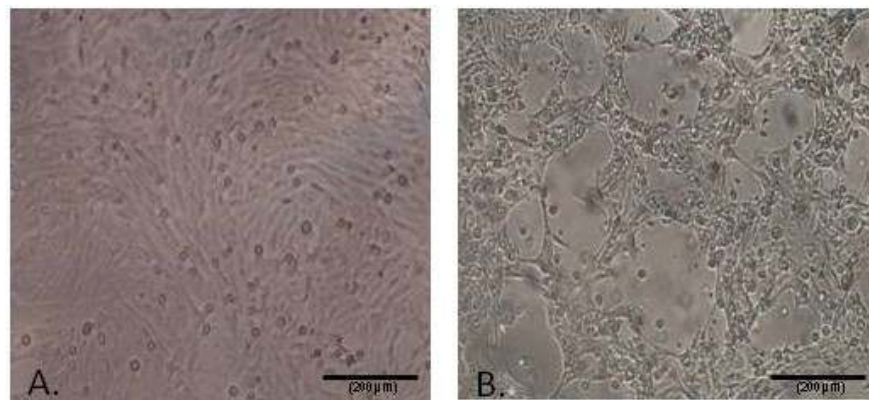


Fig.1. Influenza virus culture in MDCK cell line A. Normal cell line B. Cell line showing CPE[d5]

Although virus isolation using cell cultur~~ing~~ is considered as 'gold standard', ~~but~~ it is labour-intensive and the results depend on the optimal sample transport. Moreover, the virus can become undetectable in the later course of the infection due to decline in viable virus count with time [29-31]. Other diagnostic techniques, such as viral antigen detection and shell vial cultur~~ing~~ provide results ~~some~~-faster but generally are less sensitive than conventional cell culturing [32-35]. Rapid detection kits are also available

to detect influenza viruses and most of these tests distinguish either influenza A or influenza B but are unable to further subtype influenza A viruses. Although these rapid tests give results in less than 30 min, but the performance and reliability are the issues faced by such tests [36-39].

Molecular detection methods include conventional PCR based tests, NASBA, Real time PCR, RT-LAMP and microarray based assays. Conventional RT-PCR is successfully applied in the detection and typing of influenza viruses. In most of the ~~poor and~~ developing countries conventional RT-PCR is preferred over real time PCR due to high instrument and reagent costs of ~~the latter~~ real time RT-PCR [40-41]. In our study, standardized conventional RT-PCR detected both influenza A and B virus while no amplification was seen in negative controls. ~~Amplicons were subjected to 2.5% agarose gel electrophoresis.~~ Influenza A virus showed a strong band of 239 bp while influenza B virus showed the product band of 198 bp (**Fig. 2**).

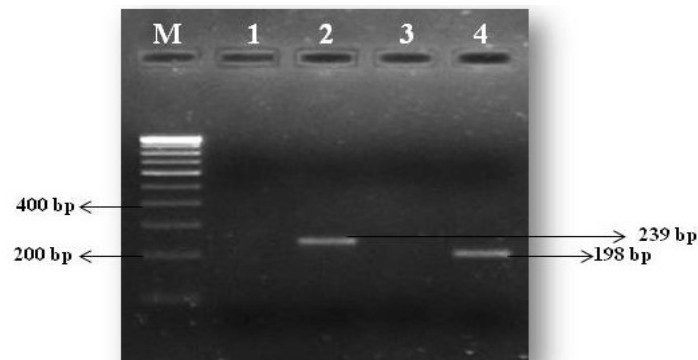


Fig. 2. Agarose electrophoresis results of conventional one step RT-PCR products. Lane M, 100 bp DNA ladder; lane 1 and 3, negative control for Influenza A and B virus respectively; lane 2 and 4, positive control for influenza A and B virus respectively.

Real time RT-PCR is rapid, sensitive and specific method for diagnosis of influenza viruses [19,20,42] and the results obtained are same ~~when compared with~~ that of virus isolation but in shorter time. Real time RT-PCR using Taqman probes is more rapid, sensitive and specific than conventional RT-PCR [42]. As Taqman probes are costly so SYBR Green based Real time RT-PCR can also be used to reduce cost, but it also compromise with the specificity of the assay. ~~In our present study, We used Taqman Real-Time RT-PCR assay to detect both Influenza A and Influenza B viruses in the reaction tubes.~~ both Influenza A and B virus showed **Ct [d6]** value of 17 (**Fig. 3**) ~~in Taqman Real-Time RT-PCR assay.~~


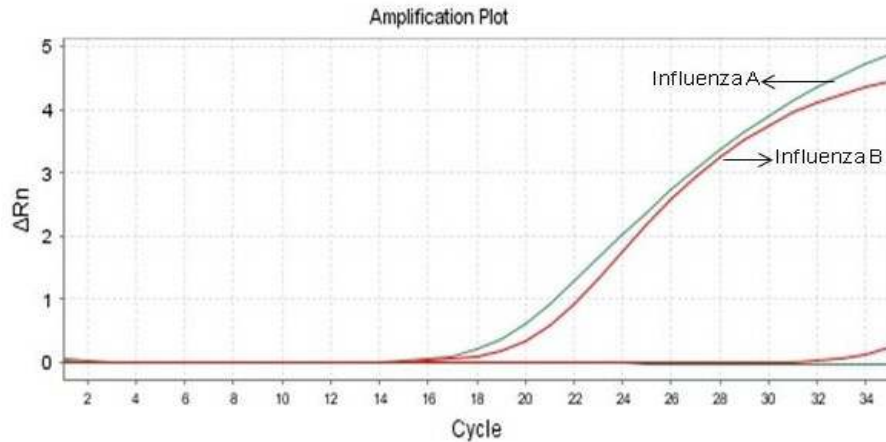


Fig. 3. Amplification curve of Taqman real time RT-PCR for Influenza A and B virus, both viruses showing Ct value 17.

Loop mediated isothermal amplification (LAMP) is an efficient method of nucleic acid amplification like PCR based methods but it amplify the target sequence under isothermal conditions. It is highly specific as four primers corresponding to six target sequences were used for amplification [43]. LAMP reaction when combined with reverse transcription i.e. RT-LAMP, has been used to detect various RNA viruses like Japanese Encephalitis, Chikungunya, Dengue, Zika virus, Norovirus, human metapneumovirus, Respiratory Syncytial virus and West Nile virus [44]. RT-LAMP can be customized for real time detection using dyes such as SYBR green or Calcein like Real Time RT-PCR, which eliminate the need of electrophoresis for analysing the results [46]. RT-LAMP assay has been applied successfully for Influenza virus detection and sub-typing [23-25,27,44-49].

In our study, RT-LAMP detected Influenza A and B virus presence in the respective tubes while no amplification was observed in negative controls, as shown in. ~~The amplicons of RT-LAMP were subjected to 2.5% agarose gel which showed the high amplification in the positive controls while there is no amplification in the negative controls (Fig. 4).~~

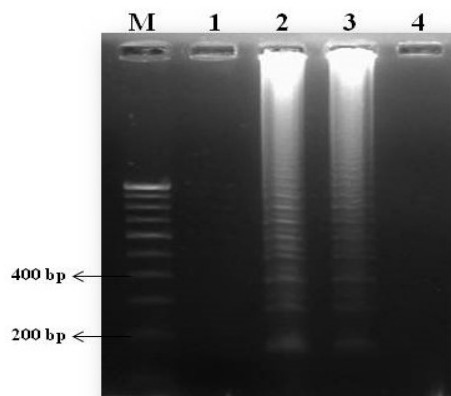

Fig[d7]. 4. Gel electrophoresis analysis of RT-LAMP products. Lane M, 100 bp DNA ladder; lane 1 and 4, negative controls for Influenza A and B virus respectively; lane 2 and 3, positive controls for influenza A and B virus respectively.

In our study, we found that all three molecular detection assays i.e. Conventional RT-PCR, Real time RT-PCR and RT-LAMP showed similar results when compared with the virus culture. All the three molecular methods are highly specific as none of these methods showed positive results with Adenoviruses, Parainfluenza viruses and RSV. Sensitivity of molecular assays was also compared and we found that RT-LAMP assay showed similar results as that of Real time RT-PCR but in less time. RT-LAMP was found to be ten times more sensitive than conventional one step RT-PCR (Fig. 5). In a the study done by of Poon et al. (2005), sensitivity of RT-LAMP was found ten times more-greater than that of conventional RT-PCR [23]. Imai et al. (2006) have reported 100 times sensitivity of RT-LAMP in comparison to RT-PCR for detecting~~ing~~-of avian influenza virus [47]. Previous studies has shown that RT-LAMP have comparable sensitivity with that of real time RT-PCR for influenza viruses [24,49].

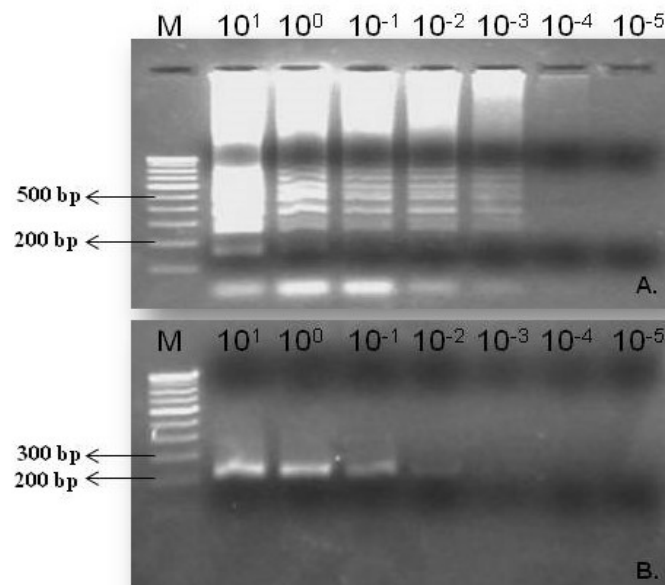


Fig. 5. Sensitivity of RT-LAMP in comparison to conventional RT-PCR. Influenza A virus strain (A/New Caledonia/20/99 (H1N1-like), with known titre of 3×10^3 PFU/ μ l, was diluted ten-fold serially and detected with RT-LAMP (gel A) and conventional RT-PCR (gel B).

4. CONCLUSION

~~Virus culture methods are labour-intensive and lengthy methods for influenza virus detection. It takes about 3-4 days to grow virus in cell lines and thereafter its detection. Conventional RT-PCR and Real time RT-PCR both are rapid, sensitive and specific diagnosis assays and detect and subtypes influenza viruses in 3-4 h when compared with virus cell culture. RT-LAMP provides the same results as that of other methods but in short time (30-60 min) and also it is less costly as there is no need of thermocycler. Only important point with RT-LAMP is design of primers as RT-LAMP assay require complex primers so if the primer designing is not accurate, it can lead to false positive or negative amplifications. [d8]~~ The current study showed that the results of molecular detection methods are same as that of virus culture and among the three molecular assays, RT-LAMP ~~method was~~ proved to be specific, sensitive, rapid and cost effective method for influenza A and B virus detection. Development of such rapid sensitive specific and cost effective assays will be useful for influenza diagnosis, early patient management, surveillance and controlling the spread of the disease.

REFERENCES

1. Michaelis M, Doerr HW, Cinatl JJr. Novel swine-origin influenza A virus in humans: another pandemic knocking at the door. *Med Microbiol Immunol*. 2009; 198(3):175-83.
2. Betts RF. Influenza virus. In: Mandell GL, Bennett JE, Dolin R, editors. *Principles and Practice of Infectious Diseases*, 4th ed. New York: Churchill Livingstone. 1995.
3. Collin EA, Sheng Z, Lang Y, Ma W, Hause BM, Li F. Cocirculation of two distinct genetic and antigenic lineages of proposed influenza D virus in cattle. *J Virol*. 2015; 89(2):1036-42.
4. Quast M, Sreenivasan C, Sexton G, Nedland H, Singrey A, Fawcett L, et al. Serological evidence for the presence of influenza D virus in small ruminants. *Vet Microbiol*. 2015; 180(3-4):281-85.
5. Song H, Qi J, Khedri Z, Diaz S, Yu H, Chen X, et al. An open receptor-binding cavity of hemagglutinin-esterase-fusion glycoprotein from newly-identified Influenza D Virus: Basis for its broad cell tropism. *PLoS Pathog*. 2016; 12(1):e1005411.
6. Cox NJ, Subbarao K. Global epidemiology of influenza: past and present. *Annu Rev Med*. 2000; 51:407-21.
7. Anonymous. Types of Influenza viruses. Centers for Disease Control and Prevention. Accessed 22 June 2016.
Available: <http://www.cdc.gov/flu/about/viruses/types.htm>.
8. Webster RG, Bean WJ, Gorman OT, Chambers TM, Kawaoka Y. Evolution and ecology of influenza A viruses. *Microbiol Rev*. 1992; 56(1):152-79.

9. Olsen B, Munster VJ, Wallensten A, Waldenstrom J, Osterhaus AD, Fouchier RA. Global patterns of Influenza A virus in wild birds. *Science*. 2006; 312:384-88.
10. Merchant GL, Mower WR, Talan DA. Update on emerging infections from the Centers for Disease Control and Prevention. Influenza: ED considerations for the 1997-98 seasons. *Ann Emerg Med*. 1997; 30:692-694.
11. Brammer TL, Murray EL, Fukuda K, Hall HE, Klimov A, Cox NJ. Surveillance for influenza-United States, 1997-98, 1998-99, and 1999-00 seasons. *MMWR Surveill Summ*. 2002; 51(7):1-10.
12. Centres for Disease Control and Prevention. Emergence of avian influenza A(H7N9) virus causing severe human illness-China, February-April 2013. *MMWR*. 2013; 62(18):366-71.
13. Anonymous. Influenza (Seasonal). Fact Sheet No. 211. World Health Organization. 2014. Accessed 23 June 2016.
Available: <http://www.who.int/mediacentre/factsheets/fs211/en/>.
14. Anonymous. WHO Global Influenza Surveillance Network (GISN). WHO Collaborating Centre for Reference and Research on Influenza. Accessed 22 June 2016.
Available: http://www.influenzacentre.org/centre_GISN.htm.
15. Takimoto S, Grandien M, Ishida MA, Pereira MS, Paiva TM, Ishimaru T, et al. Comparison of enzyme-linked immunosorbent assay, indirect immunofluorescence assay, and virus isolation for detection of respiratory viruses in nasopharyngeal secretions. *J Clin Microbiol*. 1991; 29(3):470-74.
16. Ge Y, Cui L, Qi X, Shan J, Shan Y, Qi Y, et al. Detection of novel swine origin influenza A virus (H1N1) by real-time nucleic acid sequence-based amplification. *J Virol Methods*. 2010; 163(2):495-97.
17. Zhang WD, Evans DH. Detection and identification of human influenza viruses by the polymerase chain reaction. *J Virol Methods*. 1991; 33(1-2):165-89.
18. Pregliasco F, Mensi C, Camorali L, Anselmi G. Comparison of RT-PCR with other diagnostic assays for rapid detection of influenza viruses. *J Med Virol*. 1998; 56(2):168-73.
19. Spackman E, Suarez DL. Type A influenza virus detection and quantitation by real-time RT-PCR. *Methods Mol Bio*. 2008; 436:19-26.
20. Carr MJ, Gunson R, Maclean A, Coughlan S, Fitzgerald M, Scully M, et al. Development of a real-time RT-PCR for the detection of swine-lineage influenza A (H1N1) virus infections. *J Clin Virol*. 2009; 45(3):196-99.
21. Li J, Chen S, Evans DH. Typing and subtyping influenza virus using DNA microarrays and multiplex reverse transcriptase PCR. *J Clin Microbiol*. 2001; 39(2):696-04.
22. Dawson ED, Moore CL, Dankbar DM, Mehlmann M, Townsend MB, Smagala JA, et al. Identification of A/H5N1 influenza viruses using a single gene diagnostic microarray. *Anal Chem*. 2007; 79(1):378-84.

23. Poon LL, Leung CS, Chan KH, Lee JH, Yuen KY, Guan Y, et al. Detection of human influenza A viruses by loop-mediated isothermal amplification. *J Clin Microbiol.* 2005; 43(1):427-30.
24. Parida M, Shukla J, Sharma S, Ranghia Santhosh S, Ravi V, Mani R, et al. Development and evaluation of reverse transcription loop-mediated isothermal amplification assay for rapid and real-time detection of the swine-origin influenza A H1N1 virus. *J Mol Diagn.* 2011; 13:100-07.
25. Kubo T, Agoh M, Mai le Q, Fukushima K, Nishimura H, Yamaguchi A, et al. Development of a reverse transcription-loop-mediated isothermal amplification assay for detection of pandemic (H1N1) 2009 virus as a novel molecular method for diagnosis of pandemic influenza in resource-limited settings. *J Clin Microbiol.* 2010; 48(3):728-35.
26. Anonymous. WHO information for molecular diagnosis of influenza virus-update. World Health Organization. 2014. Accessed 18 December 2015.
Available: http://www.who.int/influenza/gisrs_laboratory/molecular_diagnosis/en/.
27. Ito M, Watanabe M, Nakagawa N, Ihara T, Okuno Y. Rapid detection and typing of influenza A and B by loop-mediated isothermal amplification: comparison with immunochromatography and virus isolation. *J Virol Methods.* 2006; 135(2):272-75.
28. Van Elden LJR, Nijhuis M, Schipper P, Schuurman R, van Loon AM. Simultaneous Detection of Influenza Viruses A and B Using Real-Time Quantitative PCR. *J Clin Microbiol.* 2001; 39(1):196-200.
29. Hayden FG, Osterhaus ADME, Treanor JJ, Fleming DM, Aoki FY, Nicholson KG, et al. Efficacy and safety of the neuraminidase inhibitor zanamivir in the treatment of influenza virus infections. *N Engl J Med.* 1997; 337(13):874-80.
30. Wibawa H, Henning J, Waluyati DE, Usman TB, Lowther S, Bingham J, et al. Comparison of serological assays for detecting antibodies in ducks exposed to H5 subtype avian influenza virus. *BMC Vet Res.* 2012; 8:117.
31. Dong L, Hong B, Tian B, Rongbao G, Dong J, Zhang Y, et al. A combination of serological assays to detect human antibodies to the Avian Influenza A H7N9 virus. *PloS one.* 2014; 9(4):e95612.
32. Doller G, Schuy W, Tjhen KY, Stekeler B, Gerth HJ. Direct detection of influenza virus antigen in nasopharyngeal specimens by direct enzyme immunoassay in comparison with quantitating virus shedding. *J Clin Microbiol.* 1992; 30(4):866-69.
33. Ziegler T, Hall H, Sanchez-Fauquier A, Gamble WC, Cox NJ. Type and subtype specific detection of influenza viruses in clinical specimens by rapid culture assay. *J Clin Microbiol.* 1995; 33(2):318-21.
34. Schmid M L, Kudesia G, Wake S, Read RC. Prospective comparative study of culture specimens and methods in diagnosing influenza in adults. *Br Med J.* 1998; 316(7127):275.
35. Leland DS, Ginocchio CC. Role of cell culture for virus detection in the age of technology. *Clin Microbiol Rev.* 2007; 20(1):49-78.

36. Drexler JF, Helmer A, Kirberg H, Reber U, Panning M, Muller M, et al. Poor clinical sensitivity of rapid antigen test for influenza A pandemic (H1N1) 2009 virus. *Emerg Infect Dis.* 2009; 15(10):1662-64.
37. Cruz AT, Demmler-Harrison GJ, Caviness AC, Buffone GJ, Revell PA. Performance of a rapid influenza test in children during the H1N1 2009 influenza a outbreak. *Pediatrics.* 2010; 125(3):e645-50.
38. Gordon A, Videia E, Saborio S, Lopez R, Kuan G, Balmaseda A, et al. Diagnostic accuracy of a rapid influenza test for pandemic influenza A H1N1. *PLoS One.* 2010; 5(4):e10364.
39. Chartrand C, Leeflang MM, Minion J, Brewer T, Pai M. Accuracy of rapid influenza diagnostic tests: A meta-analysis. *Ann Intern Med.* 2012; 156(7):500-11.
40. Ieven M. Currently used nucleic acid amplification tests for the detection of viruses and atypicals in acute respiratory infections. *J Clin Virol.* 2007; 40(4):259-76.
41. Simmerman JM, Uyeki TM. The burden of influenza in East and South-East Asia: a review of the English language literature. *Influenza Other Respir Viruses.* 2008; 2(3):81-92.
42. Lopez RP, Catalan P, Giannella M, Garcia de Viedma D, Sandonis V, Bouza E. Comparison of real-time RT-PCR, shell vial culture, and conventional cell culture for the detection of the pandemic influenza A (H1N1) in hospitalized patients. *Diagn Microbiol Infect Dis.* 2011; 69(4):428-31.
43. Notomi T, Okayama H, Masubuchi H, Yonekawa T, Watanabe K, Amino N, et al. Loop-mediated isothermal amplification of DNA. *Nucleic Acids Res.* 2000; 28(12):E63.
44. Parida M, Sannarangaiah S, Dash PK, Rao PV, Morita K. Loop mediated isothermal amplification (LAMP): a new generation of innovative gene amplification technique; perspectives in clinical diagnosis of infectious diseases. *Rev Med Virol.* 2008; 18(6):407-21.
45. Bao H, Zhao Y, Wang Y, Xu X, Shi J, Zeng X, et al. Development of a Reverse Transcription Loop-Mediated Isothermal Amplification method for the rapid detection of Subtype H7N9 Avian Influenza virus. *Biomed Res Int.* 2014; 2014:525064.
46. Luo S, Xie Z, Xie L, Liu J, Xie Z, Deng X, et al. Reverse-transcription, loop-mediated isothermal amplification assay for the sensitive and rapid detection of H10 subtype avian influenza viruses. *Virol J.* 2015; 12:145.
47. Imai M, Ninomiya A, Minekawa H, Notomi T, Ishizaki T, Tashiro M, et al. Development of H5-RT-LAMP (loop-mediated isothermal amplification) system for rapid diagnosis of H5 avian influenza virus infection. *Vaccine.* 2006; 24(44-46):6679-82.
48. Jayawardena S, Cheung CY, Barr I, Chan KH, Chen H, Guan Y, et al. Loop-mediated isothermal amplification for influenza A (H5N1) virus. *Emerg Infect Dis.* 2007; 13(6):899-901.
49. Dinh DT, Le MT, Vuong CD, Hasebe F, Morita K. An Updated Loop-Mediated Isothermal Amplification Method for Rapid Diagnosis of H5N1 Avian Influenza Viruses. *Trop Med Health.* 2011; 39(1):3-7.