

# Use of Ultrasound and Anterior Segment Optical Coherence Tomography to compare Central Corneal Thickness values in patients with Open Angle Glaucoma

## ABSTRACT

**Purpose:** To compare central corneal Thickness (CCT) using ultrasound (US) pachymetry and Anterior Segment Optical Coherence Tomography (AS-OCT), in patients with open-angle glaucoma (OAG).

**Methods:** Ninety patients above 50 years with healthy corneas were prospectively included for repeated measurements of central corneal Thickness (CCT), using ultrasound pachymetry (US) and Anterior Segment Optical Coherence Tomography (AS-OCT), during the same visit. The readings were averaged and compared by paired t-test. Both eyes of each participant were measured for our study.

**Results:** Ultrasound pachymetry showed significantly higher CCT values. The CCT measured by AS-OCT and ultrasound was  $525 \pm 32.1 \mu\text{m}$  and  $533 \pm 38 \mu\text{m}$  respectively for the right eye. For the left eye the values were  $523 \pm 31.2 \mu\text{m}$  and  $532 \pm 33.1 \mu\text{m}$  respectively for the AS-OCT and US. The difference in CCT measurement by AS-OCT and ultrasound was statistically significant ( $P < 0.001$ ) in both eyes with mean standard deviation of ultrasound CCT being  $16.14 \mu\text{m}$  greater than the mean of AS-OCT CCT for the right and  $15.12 \mu\text{m}$  for the left eye. A strong correlation was found ( $r > 0.80$ ) between the CCT measurement techniques. The Anova test didn't reveal serious differences neither with AS-OCT, nor with US pachymetry.

**Conclusion:** The AS-OCT is a promising non-contact and reproducible equipment that is comparable to ultrasound pachymetry. The CCT measurement by ultrasound pachymetry gives higher values compared to AS-OCT measurement in patients with OAG. Hence, they cannot be interchangeably used in clinical practice and both must be considered.

**Keywords:** Primary open-angle glaucoma, pachymetry, central corneal thickness, Anterior Segment Optical Coherence Tomography.

## 1. INTRODUCTION


For the past years the clinical gold standard for glaucoma follow up is the measurement of the Intraocular Pressure (IOP). It has been shown that central corneal thickness (CCT) significantly affects IOP measurement and may be itself a risk factor for developing glaucoma<sup>1-5</sup>.

CCT is also a predictive factor for glaucoma progression in patients with higher than normal Intraocular Pressure. Since IOP measurement by applanation tonometry is influenced by CCT, it is important to obtain a reliable corneal pachymetry value for each patient with

23 glaucoma and adjust the IOP for the measured CCT <sup>6,7</sup>. There are many techniques  
 24 available to measure CCT. Two of the most reliable are ultrasound, and anterior segment  
 25 optical coherence tomography (AS-OCT).  
 26 During the last years ultrasound pachymetry has being incorporated into everyday practice  
 27 as a screening tool, for it is easy and convenient to repeat several measurements.  
 28 Ultrasound pachymetry is a contact procedure.  
 29 On the other hand, AS-OCT devices use a non-contact procedure, that detects minute  
 30 differences in tissue depth and they provide high-resolution cross-sectional imaging of the  
 31 cornea. Studies among non-glaucoma patients have confirmed that AS-OCT has an  
 32 acceptable level of correlation with ultrasonic pachymetry although the two methods are not  
 33 interchangeable <sup>8,9</sup>.  
 34 The purpose of this study was to investigate if the same happens in open angle glaucoma  
 35 patients.

## 37 2. MATERIAL AND METHODS

38  
 39 Hundred and eighty eyes were prospectively included in this study. Exclusion criteria  
 40 included patients with any corneal pathology such as pterygium or ectasias, previous  
 41 surgical intervention and any type of glaucoma other than OAG. All patients by the time of  
 42 the study were under latanoprost therapy for a month, but did not take any antiglaucoma  
 43 medication before our study and they were new patients.  
 44 All patients undergone ophthalmologic examination in the slit lamp, where fundus was  
 45 examined and intraocular pressure (IOP) was measured. Refractive examination was also  
 46 done. None had any significant spherical or cylindrical error and all measurements were  
 47 made between 17.00h and 20.00h the same day by the same observer. Visante AS - OCT  
 48 measurements were carried out first using the global pachymetry function. Patients' eye was  
 49 aligned after head stabilization and cross-sectional images were obtained. Visante software  
 50 processes the image and calculates automatically the map. The map is divided into eight  
 51 zones: superior, temporal, superior temporal, inferior temporal, inferior, nasal, inferior nasal,  
 52 superior nasal, and four rings of 2mm, 5mm, 7mm and 10mm diameter. Mean, maximum  
 53 and minimum values of CCT were recorded.  
 54 (Figure 1.)

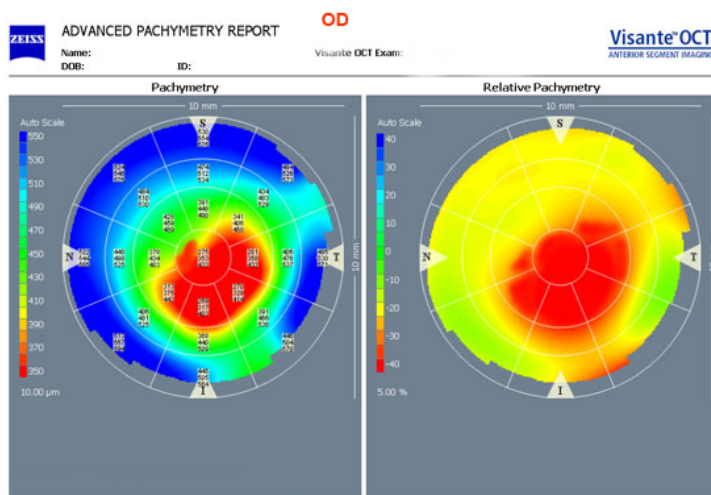

55  
 56 **Figure 1. Visante AS-OCT (anterior segment optical coherence tomography)**

57 **global pachymetric map.**

58

59 Pachymetry was then performed using the NIDEK US – 1800 ultrasonic pachymeter after  
60 applying a topical anesthetic. Prior to the measurement, the US pachymeter was calibrated  
61 according to the manufacturer's instructions. A-scan velocity was set at 1640 m/s for all  
62 measurements. The above series of exams was strictly observed to keep the epithelium of  
63 the cornea intact. As per protocol two AS-OCT and ten US separate consecutive CCT  
64 measurements were obtained. The patient's age ranged from fifty to sixty-five years.

65

## 66 **2.1 Statistical analysis**

67

68 All statistical analyses were performed using SPSS 15.0 software. SPSS is a comprehensive  
69 system for analyzing data. It takes data and generates reports, charts, descriptive statistics  
70 and plots of distribution. A p-value less than 0.05 was considered statistically significant. In  
71 the statistical analysis the mean value of the measurements was used.

72 The agreement of CCT measured by AS-OCT and Ultrasound pachymetry was compared by  
73 paired t-test. Pearson test was also used to compare correlation between AS-OCT and  
74 Ultrasound.

75 We used the Bland-Altman method to calculate the mean and 95 per cent limits of  
76 agreement (LOA) <sup>10,11</sup> and to evaluate the agreement between the two methods.

77

## 78 **3. RESULTS**

79

80 Hundred and eighty eyes were enrolled in this study. There were 40 males and 50 females.  
81 Average age of the subjects was 51 ± 9 years and there were no significant differences in  
82 terms of age and gender. The age-sex distribution of the subjects is shown in Table 1.

83 **Table 1. Demographic data**

84

|                           |    |
|---------------------------|----|
| <b>Number of patients</b> | 90 |
| <b>Age (mean)</b>         | 55 |
| <b>Male</b>               | 40 |
| <b>Female</b>             | 50 |

85

86 All subjects were treated with latanoprost and they were new patients, participating in the  
87 study about a month after the beginning of their treatment. From the statistical analysis a  
88 positive correlation was observed between the measurements of AS-OCT and US.  
89 (P<0.001).

90 Central cornea thickness was measured and the result was 525 ± 32.1µm with AS-OCT and  
91 533 ± 38 µm for US pachymetry. For the left eye the values were 523 ± 31.2 µm and 532 ±  
92 33.1 µm respectively for the AS-OCT and US. (Table 2)

93

94 **Table 2. CCT as measured with AS-OCT and US**

95


|                         | <b>Min value</b> | <b>Max value</b> | <b>Mean value</b> <sup>96</sup> |
|-------------------------|------------------|------------------|---------------------------------|
| <b>AS-OCT right eye</b> | 525 µm           | 557 µm           | 541 µm                          |
| <b>US right eye</b>     | 533 µm           | 571 µm           | 552 µm                          |
| <b>AS-OCT left eye</b>  | 523 µm           | 554 µm           | 538 µm                          |
| <b>US left eye</b>      | 532 µm           | 565 µm           | 548 µm                          |

97 From the statistic analysis with paired t-test we concluded that the differences between the  
98 two instruments was  $9.90 \pm 7.34 \mu\text{m}$  and  $9.70 \pm 7.12$  for the right and left eyes. (Table 3).  
99

100  
101 **Table 3. Difference in CCT with paired t-test between the AS-OCT and US in both eyes.**  
102

| Paired t-test CCT     | Mean value  | P      |
|-----------------------|-------------|--------|
| US – AS-OCT right eye | 9.90 (7.34) | <0.001 |
| US – AS-OCT left eye  | 9,70 (7.12) | <0.001 |

103  
104  
105 The Bland–Altman analyses of the data is displayed in Figure 2 and Figure 3. From the  
106 graph we can see that agreement limits are from  $-4.54$  to  $25.10$  and from  $-4.51$  to  $25.20$   
107 for the left and right eye respectively. The mean difference of measurements between the  
108 two methods was  $9.90 \mu\text{m}$  and  $9.70$  for the right and left eyes, comparing AS-OCT and  
109 ultrasound pachymetry. We observe a greater discrepancy of the measurements between  
110 the two instruments above the value of about  $520 \mu\text{m}$  in both eyes, whereas below this value  
111 there is a better agreement and a smaller difference.  
112 The correlation of central corneal thickness with age was  $-0.078$  ( $P > 0.05$ ) for AS-OCT  
113 and  $-0.108$  ( $P > 0.05$ ) for US.  
114  
115

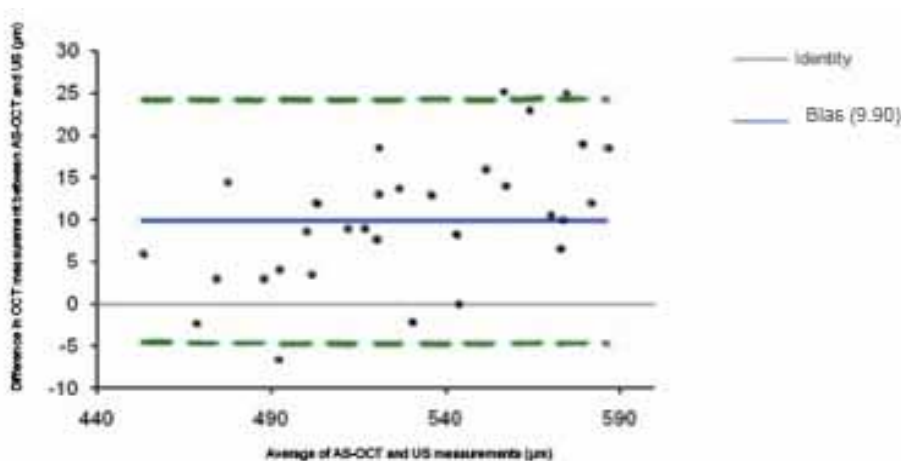

116  
117  
118 **Figure 2. Bland–Altman plot of AS-OCT and US, (right eye), showing a mean**  
119 **difference of  $9.90 \mu\text{m}$ , LOA (Limits Of Agreement) -  $4.54$  to  $+25.1 \mu\text{m}$**   
120  
121

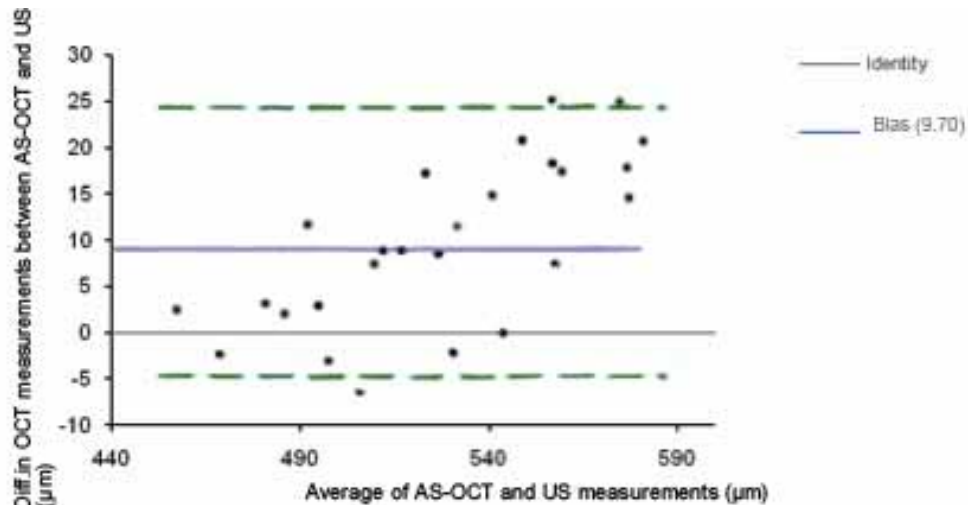


**Figure 3. Bland–Altman plot of AS-OCT and US, (left eye), showing a mean difference of 9.70  $\mu\text{m}$ , LOA (limits of agreement) - 4.51 to +25.2  $\mu\text{m}$**

### 3.1 DISCUSSION

According to the results of our study, measurements of CCT taken by AS-OCT differ significantly from the ultrasonic method. Bland–Altman Plots revealed that measurements using the AS-OCT were lower than with ultrasound, with mean difference of 9.88 mm. Repeatability of the measurements using AS-OCT was as good as with US. The repeatability of the two machines has been confirmed by other studies.<sup>12-15</sup> Central corneal thickness after statistic analysis was found to be  $525 \pm 32.1 \mu\text{m}$  with AS-OCT and  $530 \pm 38 \mu\text{m}$  with ultrasound pachymetry. The measurement of central corneal thickness with ultrasonic pachymetry is the method of choice among doctors because of its established reliability, low cost and ease of use. However, measurement by ultrasonic pachymetry requires a contact examination on the corneal epithelium and a correct technic. It is necessary to put the probe as much vertically as possible so the measurement correlates with the 2 -3 mm centrally. To have a correct measurement is also necessary to handle it with care and not force it on the cornea. Ultrasonic pachymetry is also dependent on the reflection of the sound from the anterior and posterior corneal surfaces without calculating the thickness of the tear layer that is displaced by the probe socket<sup>16</sup>. On the other hand, AS-OCT offers a non-contact mapping of the anterior surface of the cornea and a calculation of the CCT as well as high resolution imaging of the anterior chamber. Anterior segment OCT imaging was first described in 1994 by Izatt et al<sup>17</sup> using the same wavelength of light as retinal OCT, namely 830nm. This wavelength is suboptimal for imaging the angle due to limited penetration through scattering tissue such as the sclera. OCT imaging of the anterior segment with a longer wavelength of 1310 nm was developed later on and had the advantages of better penetration through sclera as well as real-time imaging at 8 frames per second. In clinical practice AS-OCT offers also an excellent qualitative and quantitative assessment of the anterior chamber and the angle and is useful as an adjunct to gonioscopy. The mean value of the measurements of CCT with AS-OCT was lower than the measurements with US in the POAG patients.

The reason for the difference between the two equipment is not completely known. It could be partly explained by the different methodology, the algorithmic differences of the two machines as mentioned above and the uncertainty about the true index of refraction of the laser light source used by AS-OCT. We must also not forget that AS-OCT offers a corneal mapping and CCT measurement in the central 2 mm. Ultrasound on the other hand offers focal on site measurement. Most of the results in previous studies comparing measurements of CCT in normal eyes, report also differences between AS-OCT and US values. One possible reason could be the number of patients participated or even the different US equipment used. In clinical practice systemic equipment errors should be considered when measuring central corneal thickness. Corneal swelling due to local anesthetic even by  $8.9\text{ }\mu\text{m}$ <sup>18,19</sup>, is another reason that we may encounter as to why AS-OCT readings may be lower than ultrasound's. We should also keep in mind that according to the Bland-Altman plots, there is a greater discrepancy of the measurements between the two instruments above the value of about  $520\text{ }\mu\text{m}$  in both eyes, whereas below this value there is a better agreement and a smaller difference. A meta-analysis by Doughty and Zaman showed that a 10% difference in the central corneal thickness could lead to a difference in intraocular pressure of up to 3.4 mmHg. They calculated that for every  $10\text{ }\mu\text{m}$  difference in the central corneal thickness, a change of 0.2 mmHg occurs in IOP measurements.<sup>20</sup> Although the difference in CCT measurements between the two equipment was less than  $20\text{ }\mu\text{m}$  in this study, the importance of CCT difference in tonometry should not be clinically ignored.

#### 4. CONCLUSION

The aim of our study was to compare Central Corneal Thickness (CCT) using ultrasound (US) pachymetry and Anterior Segment Optical Coherence Tomography (AS-OCT), in patients with open-angle glaucoma (OAG). The CCT measurement by ultrasound pachymetry gives higher values compared to AS-OCT measurement in patients with OAG. Hence, they cannot be interchangeably used in clinical practice and both must be considered. Nevertheless, further research would be useful with larger numbers of patients and longer follow-ups are required to confirm these findings and improve patient care.

#### COMPETING INTERESTS

Authors have declared that no competing interests exist.

#### CONSENT / ETHICAL APPROVAL

This study was performed with an institutional review board approval and all authors hereby declare that all experiments have been examined and approved by the appropriate ethics committee and have therefore been performed in accordance with the ethical standards laid down in the 1964 Declaration of Helsinki. After a detailed explanation of the procedure benefits and risks, consent was obtained from all patients. None of the patients refused to enroll and none were lost to follow-up during the course of the study. All authors declare that 'written informed consent was obtained from the patients for publication of this study and accompanying images. A copy of the written consent is available for review by the Editorial office/Chief Editor/Editorial Board members of this journal.

## REFERENCES

1. Argus W.A. Ocular hypertension and central corneal thickness. *Ophthalmology* 1995;102:1810-12.
2. Congdon NG, Broman AT, Bandeen-Roche K, Grover D, Quigley HA. Central corneal thickness and corneal hysteresis associated with glaucoma damage. *Am J Ophthalmol* 2006;141:868-75.
3. Herndon L, Weizer J, Stinnett S. Central corneal thickness as a risk factor for advanced glaucoma damage. *Arch Ophthalmol* 2004;122: 17-21.
4. Kohlhaas M, Boehm AG, Spoerl E, Pursten A, Grein HJ, Pillunat LE . Effect of central corneal thickness, corneal curvature, and axial length on applanation tonometry. *Arch Ophthalmol* 2006;124(4):471-6
5. Leske MC, Heijl A, Hyman L, Bengtsson B, Dong L, Yang Z, et al. Predictors of long-term progression in the early manifest glaucoma trial. *Ophthalmology* 2007;114:1965-72.
6. Ortiz S, Mena L, Rio-San Cristobal A, Martin R. Relationships between central and peripheral corneal thickness in different degrees of myopia. *Journal of Optometry*. 2014;7(1):44-50.
7. Doughty MJ, Zaman ML. Human corneal thickness and its impact on intraocular pressure measures: a review and meta-analysis approach. *Surv Ophthalmol*. 2000;44(5):367-408.
8. Doors M, Cruysberg LP, Berendschot TT, de Brabander J, Verbakel F, Webers CA, et al. Comparison of central corneal thickness and anterior chamber depth measurements using three imaging technologies in normal eyes and after phakic intraocular lens implantation. *Graefes Arch Clin Exp Ophthalmol* 2009; 247: 1139 – 1146.
9. Wong AC, Wong CC, Yuen NS, Hui SP. Correlational study of central corneal thickness measurements on Hong Kong Chinese using optical coherence tomography, Orbscan and ultrasound pachymetry. *Eye (Lond)* 2002; 16: 715-721.
10. Bland JM, Altman DG. Statistical methods for assessing agreement between two methods of clinical measurement. *Lancet* 1986; 1(8476): 307-310.
11. Bland JM, Altman DG. Applying the right statistics: analyses of measurement studies. *Ultrasound Obstet Gynecol* 2003; 22: 85-93.
12. Li H, Leuna CK, Wong L, Cheung CY, Pang CP, Weinreb RN, Lam DS. Comparative study of ventral corneal thickness with slit-lamp optical coherence tomography and Visante optical coherence tomography. *Ophthalmology*, 2008;115:796-801.
13. Fishman GR, Pons ME, Seedor JA, Liebmann JM, Ritch R. Assessment of central corneal thickness using optical coherence tomography. *Journal of Cataract and Refractive Surgery* 2005; 31:707- 711.
14. Dada T, Sihota R, Gadia R, Aggarwal A, Mandal S, Gupta V. Comparison of anterior segment optical coherence tomography and ultrasound biomicroscopy for assessment of the anterior segment. *Journal of Cataract and Refractive Surgery*, 2007; 33:837-840.
15. Mohamed S, Lee GK, Rao SK, Wong AL, Cheng AC, Li EY. Repeatability and reproducibility of pachymetric mapping with Visante anterior segment-optical coherence tomography. *Invest Ophthalmology Visual Sciences*, 2007;48:5499-504.
16. LiEY, Mohamed S, Leung CK, Rao SK, Cheng AC, Cheung CY, et al. Agreement among 3 methods to measure corneal thickness: ultrasound pachymetry, Orbscan II and Visante Anterior Segment Optical Coherence Tomography. *Ophthalmology* 2007 Oct;114(10):1842-7

- 264 17. Izatt JA, Hee MR, Swanson EA, Lin CP, Huang D, Schuman JS, et al. Micrometer-  
265 scale resolution imaging of the anterior eye in vivo with optical coherence  
266 tomography. Arch Ophthalmol. 1994;112:1584-9  
267 18. Nam SM, Lee HK, Kim EK, Seo KY. Comparison of corneal thickness after the  
268 instillation of topical anesthetics: proparacaine versus oxybuprocaine. Cornea, 2006  
269 jan 25(1):51-4.  
270 19. Herse P, Siu A. Short-term effects of proparacaine on human corneal thickness.  
271 Acta Ophthalmology, 1992;70(6):740-4.  
272 20. Doughty MJ., Zaman ML. Human corneal thickness and its impact on intraocular  
273 pressure measures: a review and meta-analysis approach. Surv Ophthalmology,  
274 2000 Mar-Apr;44(5):367-408.  
275